

BladderScan® BVI 3000

Noninvasive Bladder Volume Instrument



Operator's Manual



BladderScan[®] BVI 3000

Noninvasive Bladder Volume Instrument

Operator's Manual

Caution: In the United States, federal law restricts this device to use by or on the order of a physician.

Table of Contents

Copyright © 2006 by Verathon Inc.

All rights reserved. No part of this User's Guide may be copied or transmitted by any method without the express written consent of Verathon Inc.

BladderScan® and Sontac® are registered trademarks of Verathon Inc.
Other products and companies named in this User's Guide may be trademarks of their respective companies.

The BladderScan® instrument documented in this manual is protected by U.S. Patent Numbers 4,926,871 and 5,235,985. The Sontac® ultrasound coupling pad described in this manual is protected by U.S. Patent Number 5,782,767. Other international patents pending.

This User's Guide is Verathon™ Part No. 0900-0383.

Information in this User's Guide may change at any time without notice. Examples described or illustrated in this User's Guide are fictitious and do not in any way represent real patient or exam data.

Verathon Inc.
21222 30th Drive SE, Suite 120
Bothell, WA 98021
800.331.2313 (US and Canada only)
425.867.1348
Fax: 425.883.2896

Verathon Medical (Europe) B.V.
Boerhaaveweg 1
3401 MN IJsselstein
The Netherlands
+31.30.68.70.570
Fax: +31.30.68.70.512

Verathon Medical (Japan) K.K.
Executive Tower Azabudai 7F
1-4-3 Azabudai
Minato-ku
Tokyo, Japan 106-0041
+81.03.3560.3501
Fax: +81.03.3560.3502

Verathon Medical (United Kingdom) Ltd.
The Granary Manor Farm Courtyard
Aston Sandford, Aylesbury
Buckinghamshire, HP17 8JB
United Kingdom
+44.1844.299.207
Fax: +44.1844.299.218

Verathon Medical (France) Sarl
BP 10039
F-67012 Strasbourg Cedex
France
+33.03.88.60.14.12
Fax: +33.03.88.60.46.87

For additional contact information, please visit our website at www.verathon.com.



0900-0383-09-60

Important Information	4
BladderScan® BVI 3000 Components.....	5
Description of the BladderScan® BVI 3000	6
Preparations for Use.....	7
Customizing the BladderScan® BVI 3000	9
Operating the BladderScan® BVI 3000.....	11
Verifying Aim.....	13
Printing Results	15
Histogram of Cost Savings.....	16
Adding a Patient ID Number and Notes	17
Print Options	18
Adjusting Preferences.....	19
Additional Features.....	21
Regular Inspection and Maintenance.....	22
Trouble Shooting	23
Warranty and Disclaimer Information.....	24
Contacting Verathon Inc.	25
Safety and Performance Summary	26
Parts and Accessories	27
Technical Description.....	27
Technical Description: Battery Charger	29
Symbol Directory	30

Important Information

Product Description The BladderScan® BVI 3000 is a B-mode ultrasonic instrument, portable and battery operated, intended for the noninvasive measurement of urinary bladder volume. A mechanical sector scanning transducer provides cross-sectional images of the bladder from twelve scan planes. Based on these images, the BladderScan® automatically calculates the estimated bladder volume in milliliters and displays it on a screen.

Notice To All Operators The BladderScan® BVI 3000 should be used only by individuals who have been trained and authorized by a physician or the institution providing patient care. All operators should read this manual prior to using the BVI 3000. Failure to comply with these instructions may compromise the performance of the instrument.

Biological Safety To date, exposure to pulsed diagnostic ultrasound has not been shown to produce adverse effects. However, ultrasound should be used only by medical professionals when clinically indicated, using the lowest exposure times possible commensurate with clinical utility.

The ultrasonic output power of the BladderScan® BVI 3000 is not user-adjustable and is limited to the minimum level necessary for effective performance. Data on acoustic output levels can be found in the section titled, "Technical Description," in this manual.

Statement of Prescription *Caution: United States Federal law restricts this instrument to use by or on the order of a physician.*

Statement of Intended Use The BladderScan® BVI 3000 projects ultrasound energy through the lower abdomen of the nonpregnant patient to obtain an image of the bladder, which is used to determine bladder volume noninvasively.

Warning: Not intended for fetal use.

Warning: Not intended for use on pregnant patients.

Warning: There is the hazard of possible explosion if the BVI 3000 instrument is used in the presence of flammable anesthetics.


Cautions The BVI 3000 should not be used on a patient with open skin or wounds in the suprapubic region.

The patient should not have a catheter in his/her bladder. This could affect the accuracy of the instrument.

Use care with suprapubic/pelvic surgery patients. Scar tissue, incisions, sutures and staples affect ultrasound transmission and reflection.

Accuracy may be affected for patients with ascites or free floating fluid in the peritoneum.

BladderScan® BVI 3000 Components

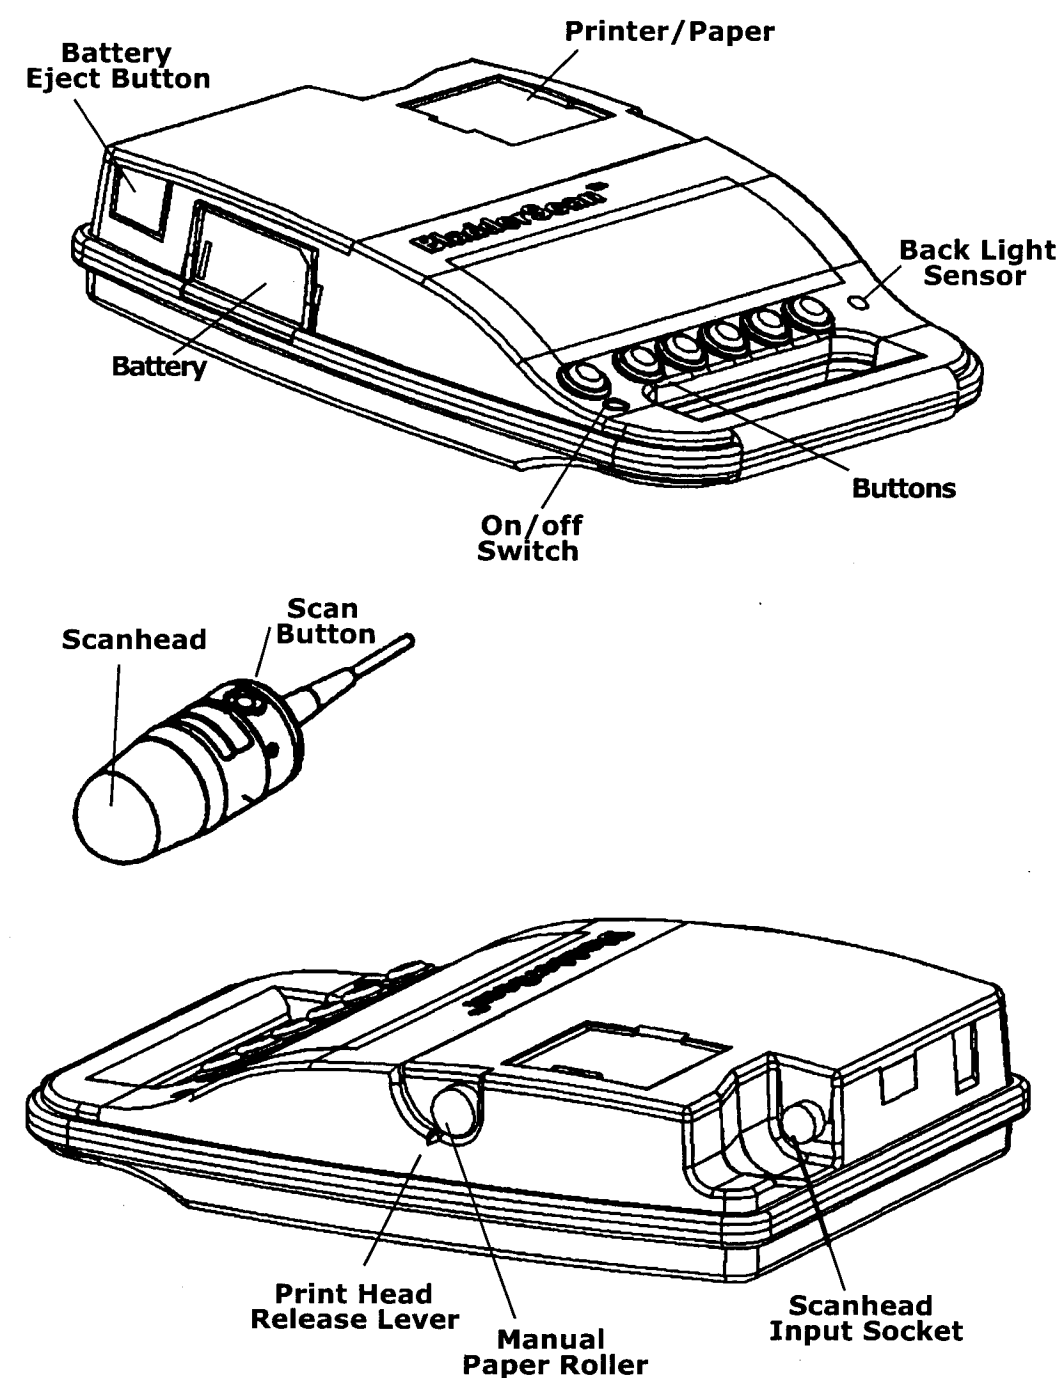

The BladderScan® BVI 3000 consists of 4 main components: The Scanhead, Control Unit, Rechargeable Battery, and Battery Charger.



Scanhead

The scanhead transmits and receives ultrasound, automatically moving its internal transducer 360° to scan twelve planes and produce a three-dimensional image of the urinary bladder. The scanhead is connected to the control unit by means of a cable.

Control Unit


The control unit provides all operating controls for the scanning procedure by means of six soft keys. The measured bladder volume and a target-shaped aiming icon are clearly displayed on the LCD screen, helping the operator to achieve accurate measurement results.

Batteries & Charger

Two NiMH rechargeable batteries are included with the BladderScan® BVI 3000. One battery can be recharged in the battery charger while the other is being used to power the BladderScan®. This ensures that there is no instrument downtime. The charger brings the battery to a full charge in 6 hours or less.

(See picture and instructions for charging the battery on page 7).


Connect the scanhead to the input socket at the back of the instrument by aligning the tabs on the scanhead plug with the matching slots on the instrument socket. Press the plug straight in until there is a "click." To remove the plug, grasp the black plastic ring and pull straight out. Do not twist.

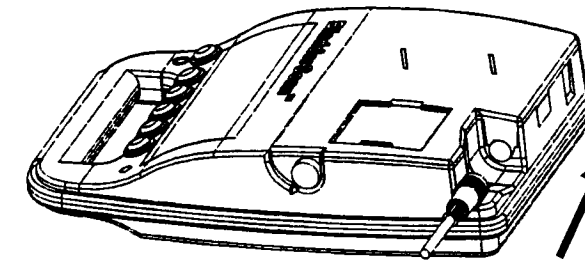

Connecting the Scanhead

To charge a battery, plug the charger into an electrical outlet. Remove the label covering the battery contacts and slip the battery into the recess on the top of the charger. Fully charging the battery may take up to 6 hours.

Batteries may be stored in the charger. There is no danger of overcharging the battery.

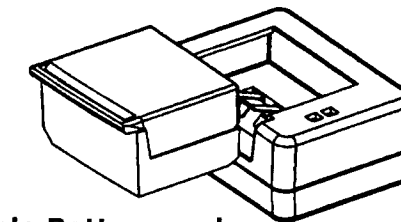

Rechargeable Battery and Battery Charger

Check the color indicator lights on top of the battery charger to determine the battery's power status while charging.

Solid Green: When the battery is low on charge, charging begins in the fast charge mode. During fast charge mode, the green light is solid. For a fully discharged battery, fast charge mode lasts about two to three hours.

Quickly Blinking Green: When the battery reaches 80% of its charge level, the charger starts to "top off" the charge and the green light blinks quickly. At this point, you can use the battery in the BladderScan® instrument.

Amber Light: In some cases the charger displays an amber light. The amber light means the battery temperature is stabilizing before recharging can begin. This may occur when the battery is taken from a very cold or warm environment, or if the battery is defective. If the light remains amber for over an hour, the battery is defective and must be replaced.

Slowly Blinking Green Light: If the green light blinks slowly upon inserting a battery, then the battery level is too low for fast charging. The charger trickle charges the battery until the power level is high enough to begin fast charging. At this point, fast charging begins automatically.

Charging Batteries


Note: The battery life is extended if you wait for about three hours until the battery is fully charged. Verathon™ recommends that you store your spare battery in the charger to prevent instrument downtime due to discharged batteries.

Note: Plugging and unplugging the charger while a battery is inserted causes no damage. There is no danger when the charger is plugged in without the battery inserted.

Installing a Battery

When the battery has been properly charged, install it in the BVI 3000 as demonstrated in the illustration below.


Battery release button

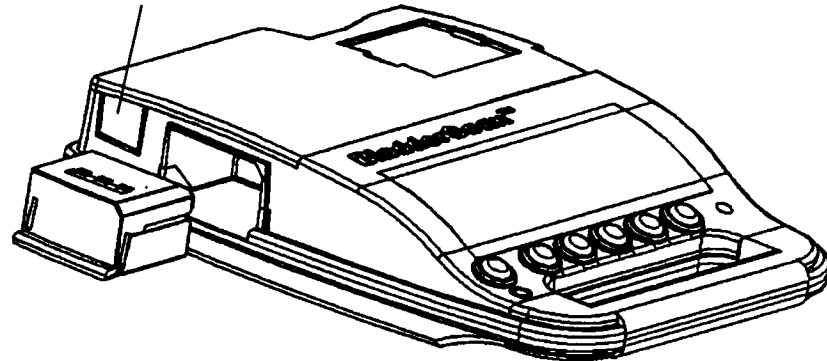

To remove the battery, push the battery release button.

Battery Icon

The battery icon, located in the upper-right corner of the BladderScan® LCD screen, indicates the power status of the battery currently installed in your instrument. Read the battery icon as follows:

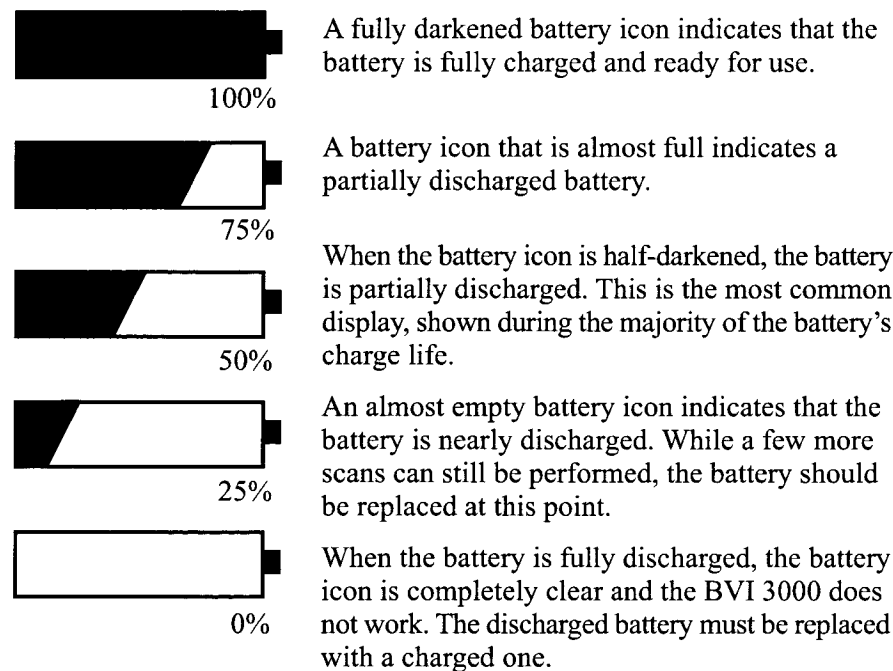


Battery Care


The BladderScan® BVI 3000 draws very little power when it is turned off; however, if you do not plan to use your instrument for several weeks, you should remove the battery to prevent it from becoming discharged.

The battery that is not in use should be stored in the charger so it remains fully charged.

Programming the Facility Name

You can customize the BladderScan® BVI 3000 instrument by entering your facility name and the current date and time. This information will subsequently be included on all printouts of exam results. To customize the BVI 3000, follow these steps:


- Turn the BVI 3000 on by pressing the button marked: 
- On the Main Menu screen, press the ALT button to display the Alternate Menu screen, illustrated below.*

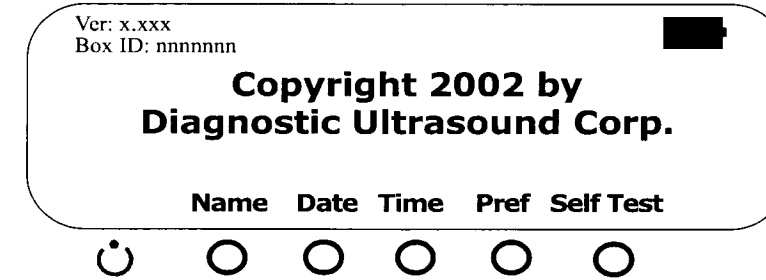

Note: Diagnostic Ultrasound Corp. is now called Verathon Inc.

***Important:** If your BVI 3000 came with the PIN code option enabled, you must enter your PIN code before you can access the Alternate Menu. The default PIN is "0000." For information about how to personalize the PIN code, see the section titled, "Adjusting Preferences," in this manual.

- Press the NAME button. The Name Preset screen, with a 4 x 13 grid containing alphabetic, numeric, and punctuation characters, is displayed.

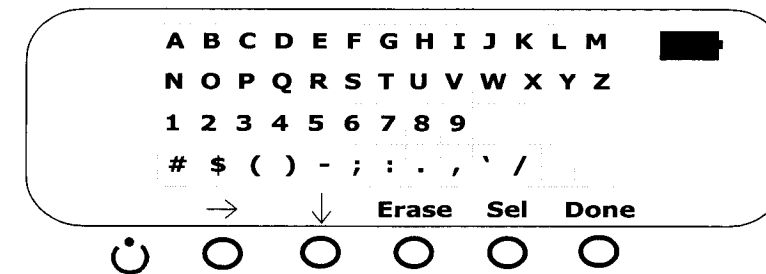

Note: You may use any combination of up to 27 characters when entering the facility name. For example, you can enter the name of the hospital, clinic, or physician supervising use of the BVI 3000.

Note: You can use the empty character as a space to separate words.


- Use the "arrow right" → and "arrow down" ↓ buttons to highlight the first character you want to enter. (To move horizontally, press the "arrow right" button. To move vertically, press the "arrow down" button).
- When you have highlighted the desired character, press the SEL button to select it. The character(s) you have selected are displayed below the character grid.
- Continue to use the "arrow right," "arrow down," and SEL buttons to enter all the characters in your facility's name. If you make a mistake, use the ERASE button to delete the last character entered.
- When you are finished, press DONE to return to the Main Menu. The programmed facility name will now be displayed on the Main Menu screen.

Note: When the arrow buttons are held down, the cursor moves one character a second. When the cursor reaches the end or bottom of the grid of characters, it wraps around to the first character again.

Setting the Date

Note: Once set, the BVI 3000 clock recognizes the number of days in each month, including February during leap years. It has its own lithium battery and maintains the correct date and time for at least ten years, even if the rechargeable battery is removed.

- On the Main Menu screen, press the ALT button to access the Alternate Menu (if prompted, enter your PIN number). Then press the DATE button.
- The Date Preset screen displays the current setting for the date, in U.S. format (two digits each for the month, day, and year).

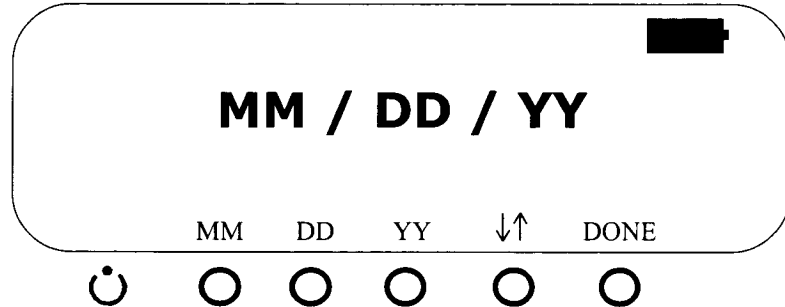


- Press the MM button until the correct month is displayed. Only values from 01 to 12 are allowed (12 is followed by 01).
- Press the DD button until the correct day is displayed. Only values from 01 to 31 are allowed (31 is followed by 01).
- Press the YY button until the correct year is displayed. Only values from 97 to 19 (for 1997 to 2019) are allowed.
- Press ↓↑ to toggle between the following options: 1) values are increased, or 2) values are decreased, when the month, day, and year buttons are pressed.
- When the date is set, press DONE to return to the Main Menu screen.

Setting the Time

Note: Enter the time in 24-hour format ("military time"). To convert standard clock time to 24-hour format, after 12-noon add 12 hours to the clock time (Example: 3:00pm + 12 hours = 15:00 hours).


- On the Main Menu screen, press the ALT button (and then enter your PIN code, if required) to access the Alternate menu. Next, press the TIME button. The Time Preset screen displays the time that is currently set.

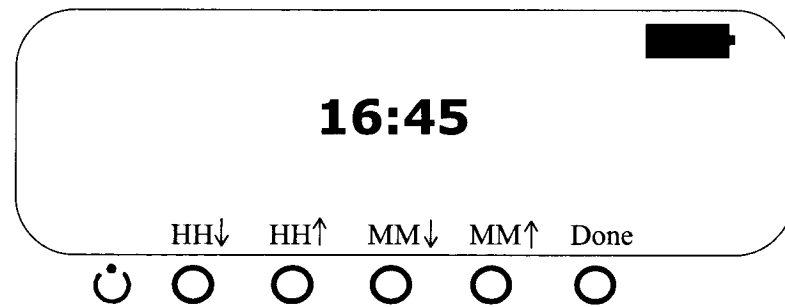


- Press the HH ↓ or HH ↑ to set the hour.
- Press the MM ↓ or MM ↑ buttons to set the minutes.
- When the time is set, press DONE to return to the Main Menu screen.


You have now customized your BladderScan® BVI 3000 instrument.

First Time Users: We advise new operators to use the BladderScan® BVI 3000 on patients with moderately full bladders, rather than initially attempting to locate nearly empty bladders. An in-service training video has been supplied with your BVI 3000. We recommend that you view the video to supplement the information in this manual with an actual demonstration of BladderScan® use.

- Turn on the BVI 3000 by pressing the button marked:  The Main Menu screen is displayed.

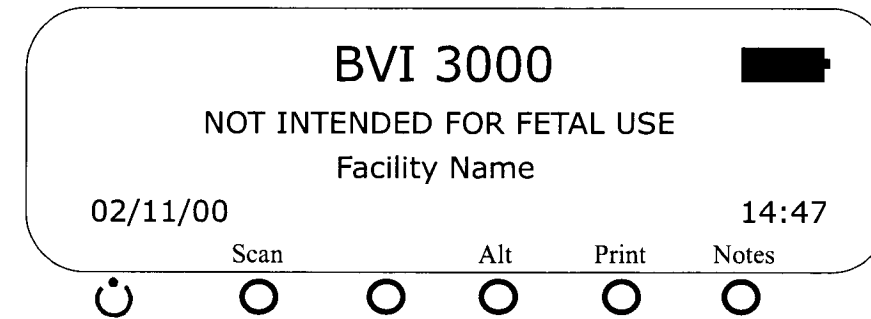

- From the Main Menu, press the SCAN button to go to the Scanning screen.

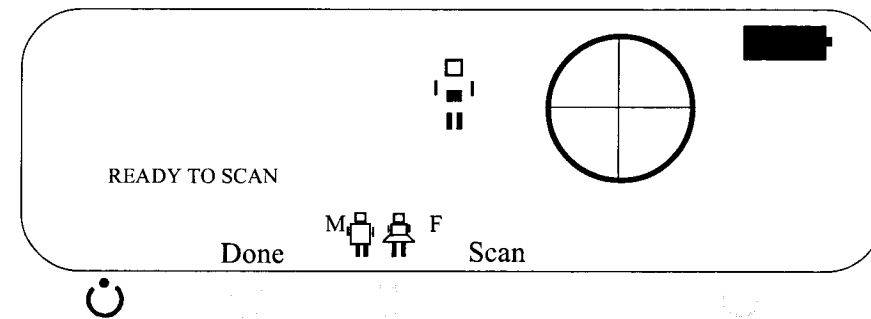

- Press the Male/Female button to select the patient gender. The LCD screen shows a male or a female icon to indicate the gender that is selected. Use the female option ONLY for women who have NOT undergone a hysterectomy (the "Female" option allows the instrument to exclude the uterus from the measurement, which may resemble the bladder ultrasonically). For all other patients, use the "Male" option.

- Clean the rounded end of the scanhead by wiping it gently with a cleaning pad dampened in isopropyl alcohol or a hospital disinfectant solution.

Turning On

Note: If the calibration due date for your BVI 3000 has passed, the message "Calibration Due" will appear every time you turn on the instrument. You can still measure bladder volume; however, this message will continue to appear until an authorized Verathon™ Service Center calibrates the instrument. Press OK to continue.


Note: The Scanning screen may also be selected by pressing the scan button on the scanhead. This is especially practical when the scanhead is already positioned on the patient's abdomen.

Selecting Gender

Preparing the Scanhead

Applying the Sontac® Ultrasound Gel Pad

The Sontac® Ultrasound Gel Pad is a convenient and easy-to-use coupling medium designed for use with the BladderScan®. To apply the Sontac® Ultrasound Gel Pad, peel back the foil lid of the individual gel pad package, exposing the gel pad. Palpate the patient's symphysis pubis (pubic bone) and place the Sontac® Gel Pad immediately superior to the patient's symphysis pubis, as shown in the images below.

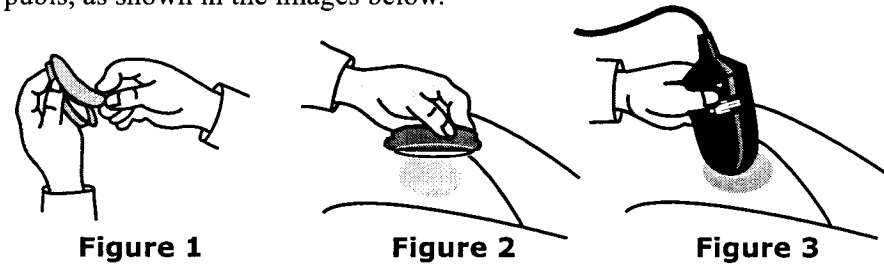


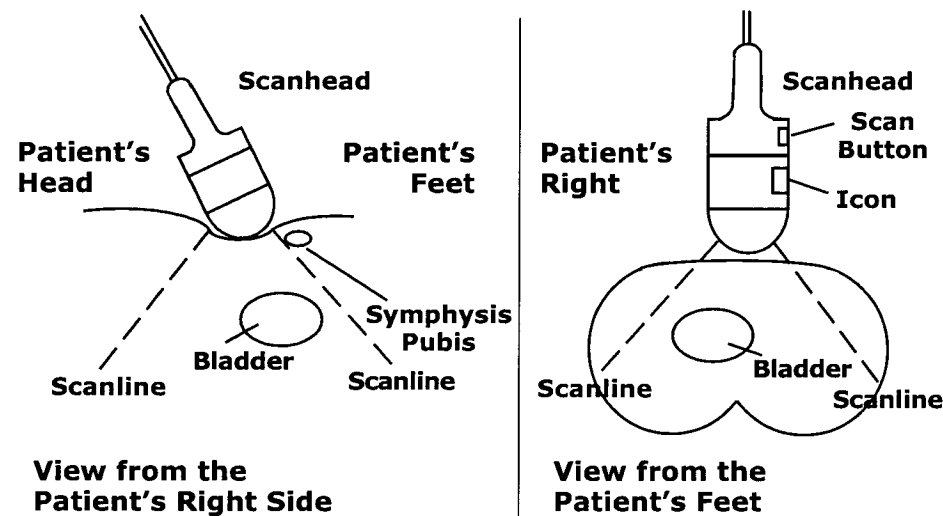
Using Ultrasound Gel


Sometimes it may be necessary to use liquid ultrasound transmission gel (for example, on obese patients or patients with excessive amounts of body hair). When using liquid ultrasound transmission gel, apply a generous amount on the round dome of the scanhead. Smooth the gel out and remove any air bubbles, which may block ultrasound transmission.

Measuring Bladder Volume

Note: While scanning, avoid making any changes in the position, angle or pressure of the scanhead.


- Locate the patient icon  on the scanhead and make sure the head of the icon will point toward the head of the patient when you place the scanhead on the patient's abdomen.
- Palpate the patient's symphysis pubis and place the scanhead midline on the patient's abdomen, approximately 1.5 inches (4 cm) superior to the symphysis pubis (see illustrations below). Or, if using Sontac® Gel Pads, simply place the scanhead on the gel pad.



- Aim the scanhead so the ultrasound is projected toward the expected location of the bladder. For most patients, this means aiming the tip of the scanhead toward the patient's coccyx.
- Press and release the scan button, located on the scanhead.  Hold the scanhead steady throughout the scan. The scanhead clicks once at each scanplane. When you hear a beep, the scan is complete. The Aiming screen is then displayed.

Aiming Screen

The greatest measured bladder volume is displayed in large type in the upper left-hand corner of the Aiming screen. Also displayed are the target-shaped Aiming Icon, the instrument status (READY TO SCAN), and the current volume measurement.

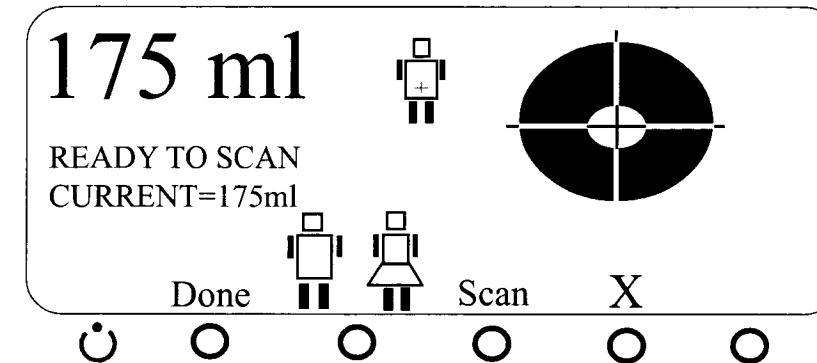

The BVI 3000 always displays two volumes; the largest volume measured and the current volume.

Largest Volume and Current Volume

We recommend that you take several measurements to ensure maximum accuracy. The BVI 3000 assumes that the largest volume measured is the true bladder volume, because in most cases the largest volume is the most accurate. Exceptions occur when the operator moves the probe during the scan, or fails to select the female gender when required. In these situations, the largest volume measurement may be higher than the actual bladder volume, and the operator should clear the aiming screen before rescanning the patient.

To clear the scan results screen, press the clear button, which is labeled with an "X" on the LCD screen. If your instrument does not have a clear button, clear the screen by pressing the DONE button and then pressing the SCAN button to start over. Then rescan your patient. In the following section, we explain how to ensure maximum accuracy by adjusting your aim.

Clearing the Screen

The light area inside the target-shaped Aiming Icon represents the position of the bladder relative to the scanhead. Accurate results are obtained when the bladder image is centered on the crosshairs of the Aiming Icon. If the bladder is not centered, re-aim the scanhead and rescan the patient. Repeat until the image is properly centered (see Figure 1).

The Aiming Icon

Adjusting Aim

The Aiming Icon displays the bladder as viewed when looking down on the patient's abdomen. To adjust your aim, slightly move or angle the scanhead toward the direction of the bladder image on the Aiming Icon (target). For example, if the bladder image is located on the right side of the icon, aim the scanhead so the ultrasound will be projected further to the right.

In Figure 1, the bladder image is centered on the crosshairs of the Aiming Icon. This indicates that the scanhead was properly aimed and the bladder volume measurement is accurate.




Figure 1

Verifying Aim (Continued)

Adjusting Aim (Continued)




Figure 2




Figure 3

In Figure 2, the bladder image is not centered on the crosshairs; the bladder overlaps one side of the Aiming Icon. This indicates that the scanhead was not properly aimed and part of the bladder was outside its field of vision. In such cases, the measured volume is lower than the true bladder volume. The BVI 3000 recognizes this condition and displays a > (greater than) symbol before the bladder volume measurement. To achieve an accurate measurement, the operator should re-aim the scanhead toward the bladder image and repeat the scan.

In Figure 3, the bladder overlaps two sides of the Aiming Icon. This indicates that the bladder is too large to be fully contained within the scanhead's field of vision. The BVI 3000 recognizes this condition and displays a > (greater than) symbol before the bladder volume measurement. In such cases, repositioning or re-aiming the scanhead will do little to improve accuracy; however, this situation arises almost exclusively in patients with very large bladder volumes. At these high volumes, measurements are clinically useful even if they underestimate the true bladder volume.


When you are satisfied that the scanhead was aimed properly and the measured bladder volume is accurate, press the DONE button. A Scan Results screen is then displayed.

The Scan Results Screen

Note: The longitudinal scan plane is marked by a gender icon bisected by a vertical line. The horizontal scan plane is marked by a gender icon bisected by a horizontal line.

The Scan Results Screen displays the longitudinal and horizontal scan planes from the **largest image** taken during the exam. The light areas represent the bladder. The dark, triangular surfaces, called scan planes, represent the scanhead's field of vision. The volume measurement is accurate when the light colored bladder images are completely contained within the dark, triangular scan planes.


If the light surface in either scan plane is overlapping the edge of the black area, or appears to be cut off, then part of the bladder was not contained in the scanhead's field of vision and the measurement may underestimate the patient's bladder volume. Press the SCAN button to clear the results of the last scan and return to the Scanning screen. Reposition the scanhead and repeat the scanning procedure.

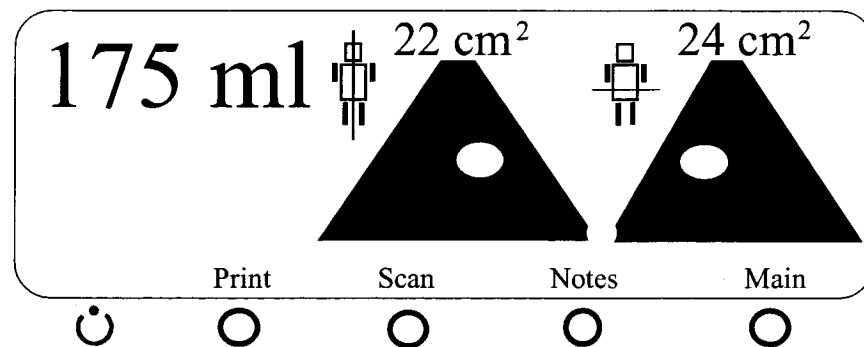

When the bladder images are completely contained in both scan planes, the measurement results are accurate. Pressing either the PRINT or MAIN button completes the scanning procedure and stores the measurement results in the instrument's memory.

Printing Results

If a printout of the scan result is desired, press the PRINT button to open the Print Menu. The Print Menu is shown below.

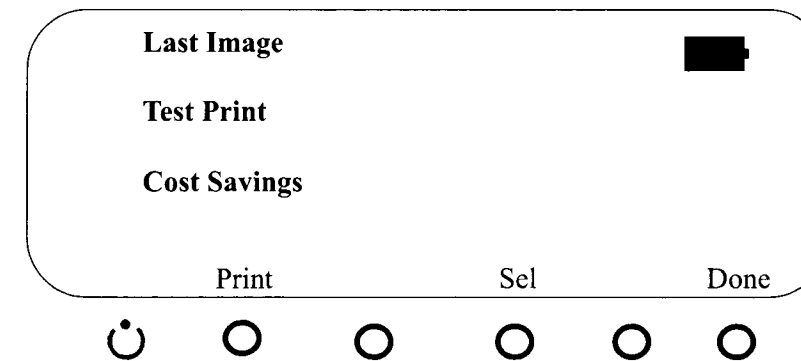


Press PRINT to obtain a printout of the most recent exam. Printing takes about one minute. See Figure 4 for an illustration of the printout.

More information about printing can be found in the "Print Options" section of this manual. During printing, the message, "Printing in Progress," is displayed. If you need to stop a print in progress, press the ABORT PRINT button.

Note: If the facility name, date, and time have not been set, those lines will be skipped on the printout. The BVI 3000 prints on thermal paper. Over time, the thermal printout will fade. For maximum storage life, we recommend that you photocopy the printout.

Figure 4

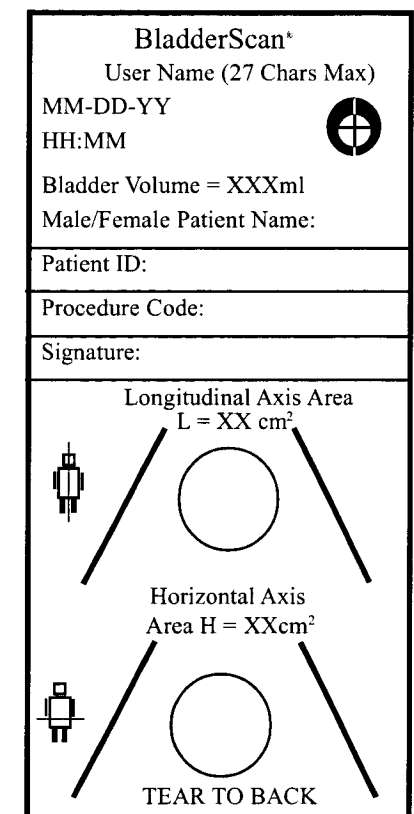

Histogram of Cost Savings

Note: The default settings can be changed in the Preference screen to reflect the rates and costs at your facility. For more information, see the section titled, "Adjusting Preferences," in this manual.

Note: For reference articles on UTI Rate and UTI Costs, see the section titled, "For Further Information," in this manual.

Figure 5

HISTOGRAM	
Volume	# of Scans
000-099	870
100-199	1,219
200-299	589
300-399	488
400-499	252
500-599	176
600-699	154
700-799	87
800-899	69
900-999	5
>1000	4
Catheterizations Avoided: 2089	
UTIs Avoided: 63	
Savings: \$49,107	

Each volume measurement from a completed scanning procedure is stored in the instrument's memory. Measurement data is stored in one of eleven volume ranges (each with a 100ml increment). This data is analyzed and can be printed at any time in a Histogram of Cost Savings (see Figure 5).

Cost savings are calculated based on the following criteria:

Catheterizations Avoided - Urinary catheterization below a certain volume is deemed unnecessary. Thus, by using the BVI 3000, these catheterizations are avoided. The default setting (for volume below which catheterization is unnecessary) is 200ml.

UTI's Avoided - Studies indicate that a certain percentage of catheterizations lead to urinary tract infections (UTI's). By avoiding unnecessary catheterizations, the resulting UTI's may be prevented. The default setting (for percent of catheterizations leading to UTI's) is 3%.

Associated Costs:

Cost of UTI's Avoided - Literature suggests that the additional costs associated with treating UTI amount to \$680.00 per patient infection. The default setting is \$680.00.

Cost of Catheter Kits - The default setting is \$3.00 (per kit).

Total Cost Savings as a Result of Using the BVI 3000:

$(\text{Caths Avoided} \times \text{Catheter Costs}) + (\text{UTI's Avoided} \times \text{UTI Costs})$

Adding a Patient ID Number and Notes

Adding a Patient ID Number

Note: Only press the button marked # when a patient ID number is required. If the # button is used and no patient ID number is entered, the BVI 3000 will assume a patient ID number was entered and 0000000000 will be printed on the printout.

A patient ID number (maximum 10 digits) can be added to the scan result and will be included on the printout. To add a patient ID number, press the button marked with a # symbol on the Scan Results screen. The screen displays 0000000000.

- Use the ← (arrow left) and → (arrow right) buttons to select the digit you want to change (the selected digit is underlined).
- Use the + (plus) or - (minus) buttons to select the correct number.
- Continue to use the ← (arrow left) and → (arrow right) buttons and the + (plus) or - (minus) buttons to enter all the digits of the patient ID number.
- When the patient ID number has been entered, press the DONE button to return to the Scan Results screen.

The patient ID number will be included on the printout of the scan.

After a scanning procedure has been completed, it is possible to annotate the measurement results. Press the button marked NOTES on the Scan Results screen. When the Notes option is selected, notes appear on the printout of the exam data.

The operator can change the following settings to annotate the exam:

Exam Type

Default settings:

- If the measured bladder volume is less than 100ml, the BVI 3000 assumes the measurement was taken after patient voiding and "POSTVOID" is displayed on the screen.
- If the measured bladder volume is between 100ml and 400ml, the BVI 3000 assumes the measurement was taken prior to patient voiding and "PREVOID" is displayed on the screen.
- If the measured bladder volume is greater than 400ml, the BVI 3000 assumes the measurement was taken prior to patient voiding and the bladder was filled to maximum capacity. "CAPACITY" is displayed on the screen.

If the default does not apply, the Exam Type setting can be changed by pressing the EXAM TYPE button to toggle between options. The selected exam type will appear on the right side of the LCD screen.

Action Taken

Using the SEL button, you can also note the action taken as a result of the current bladder volume measurement. Possible selections are:

- | | |
|-----------------------|--|
| No Action: | The default selection |
| Patient Voided: | The patient was able to void |
| Patient Catheterized: | The patient's bladder was emptied using a urinary catheter |
| Allowed to Fill: | The patient's bladder was not as full as desired and voiding was postponed |

Adjusting Volume

The instrument assumes that the amount of urine voided or catheterized is equal to the volume measured by the BVI 3000 (rounded to the nearest 10ml). This value can be adjusted up or down using the buttons labeled "+" and "-".

The Print screen can be accessed by selecting PRINT, either from the Main Menu screen or from the Scan Results screen after a scan is completed. The following table describes the different print options. From the Print screen, use the “SEL” button to select a print option. An X appears in front of the option selected.

Option	Description
Last Image	This option prints the most recent measurement data on the built-in thermal printer. Different types of images can be selected from the Preference screen, using the “Printout” option. (The default is B-mode grayscale images with highlighted bladder walls).
Cost Savings	This option is used to print a Histogram of Cost Savings based on the volume history of the instrument. Cost savings are calculated based on the catheter and UTI costs avoided due to BVI 3000 use. For details, see the section titled, “Histogram of Cost Savings,” in this manual. Histogram settings can be changed in the Preference Menu (for instructions, see the section titled, “Adjusting Preferences,” in this manual).
Test Print	Select this option to test if the built-in thermal printer works. Alphanumeric characters and a simple grayscale test pattern are printed out.

Loading Paper

Tip: To verify that you are loading the paper with the thermal side down, flick your nail over the paper. If a black mark appears, this is the thermal side.

The BVI 3000 has an automatic paper loading mechanism. To load a new roll of paper, open the paper well door at the top of the instrument and insert the end of a new paper roll, with the thermal side down, into the paper input slot. The BVI 3000 senses the presence of the paper and feeds automatically (paper is forwarded through the paper eject slot in the top of the instrument).

It is important that you feed a *straight edge* into the paper feed mechanism. Cut off the first inch of a new paper roll before loading the paper.

Caution: To avoid paper jams, never fold the end of the paper roll or cut it diagonally or to a point.

Caution: If the paper does not advance, or it appears to be stuck in the printer, turn off the instrument. Lower the printhead release lever, located adjacent to the paper advance thumb wheel. Gently pull the paper backward while moving the thumb wheel counterclockwise. If the paper jam is inaccessible, contact your authorized Verathon™ Service Center or local Verathon™ distributor for service.

Adjusting Preferences

Note: If your BVI 3000 came with the PIN code option enabled, you must enter your PIN code before you can access the Alternate Menu.

Various BVI 3000 operating parameters can be customized for individual use via the preference screen. To access the Preference screen and adjust your instrument settings, go to the Main Menu and then press “ALT” to access the Alternate Menu. (If required, enter your PIN code to access the Alternate Menu. See the section below titled, “The PIN Code Option,” for more information.) Then press the “PREF” button.

On the Preference screen, a list of adjustable parameters is displayed. Use the SEL ↑ and SEL ↓ buttons to select a parameter. Use the “+” and “-” buttons to adjust the parameter value. Press DONE to save the new setting. For a description of the adjustable parameters, see the table below.

If the PIN code option is enabled, users must enter a PIN code in order to access the Alternate Menu and change instrument settings. This prevents unauthorized users from changing the instrument settings. The default PIN code is “0000.” Enter this default code the first time you access the Alternate Menu.

To personalize your PIN code, select the change PIN option on the Preference screen. The current PIN is displayed. Enter a new PIN and then press DONE.

Important: Remember your PIN code. If your existing PIN code is forgotten, only a qualified Verathon™ Service Center can reset the PIN code.

The PIN Code Option

Personalizing the PIN Code

Parameter	Range & Values	Description
Backlight	AUTO (default) ON OFF	AUTO = Backlight turns on and off automatically, depending on ambient light conditions. ON = Backlight always on. OFF = Backlight always off.
Beep Volume	0-9 (default=5)	Allows user to adjust sound volume (lower values are quieter).
Language	ENGLISH (default) DANISH DUTCH FINNISH FRENCH GERMAN ITALIAN NORWEGIAN PORTUGUESE SPANISH SWEDISH TURKISH	Specifies the language which will be used on the display and local printout.
Date	MM/DD/YY (default) DD/MM/YY YY/MM/DD	Allows the format in which the date is displayed (order of month, day and year) to be adjusted.

(continued on next page)

Parameter	Range & Values	Description
Printout	ADD_WALLS (default)	ADD_WALLS = Print grayscale B-mode images with bladder walls highlighted.
	NO_IMAGES	NO_IMAGES = Do not print any B-mode images.
	RAW_ONLY	RAW_ONLY = Print grayscale B-mode images without identifying bladder walls.
	WALLS_ONLY	WALLS_ONLY = Bladder outline only.
	12_PLANES	12 PLANE = All 12 scan planes, printed as in the ADD_WALLS mode.
UTI_rate	0-100, (default=3%)	Percentage of catheterizations which result in UTI; used in cost savings calculations.
UTI_cost	0-2000, (default=\$680)	Cost to treat a UTI; used in cost savings calculations.
Cath_cost	0-20, (default=\$3)	Cost of a catheter; used in cost savings calculations.
Cath_vol	0-1000ml, (default=300ml)	Bladder volume below which catheterization is unnecessary; used in cost savings calculations.
Flash	ON (default)	ON = Flash memory is enabled and scans are saved even if power is removed.
	OFF	OFF = Scan information is not retained if unit is turned off; however, processing time is slightly faster.
Time Zone	GMT ± 0-12	This function currently not used.
Contrast Adjust	30-63, (default=57)	Adjust display contrast ratio; the higher the value, the darker the background. <i>Note: An immediate effect is seen only when adjusting the contrast value up. Adjusting contrast down is not visible until the instrument is turned off and then on again.</i>
Currency	\$ € £ ¥ (default=blank)	Set the currency for calculating cost savings. Choose US dollars, Euros, Pounds, or Yen. When a different currency is selected, calculations are not affected.
Scan Count Screen	# of scans performed	Selecting this option allows the user to monitor instrument usage. There are two scan counters; one is resettable and one is not. Press "Clear Count" to reset the resettable counter to zero. Only a qualified Verathon™ Service Center can reset the "non-resettable counter" to zero.
Reset Histogram		Allows the user to reset the histogram to begin a new analysis of cost savings.
Change PIN		Selecting this option takes the user to a separate screen to personalize or change the PIN code. The current PIN is displayed. Enter a new PIN and then press "DONE." <i>Important: Remember your PIN code. If your existing PIN is forgotten, only a qualified Verathon™ Service Center can reset the PIN code.</i>

Self-Test

To perform an instrument test, go to the Main Menu and press the ALT button (then enter PIN code if required) to access the Alternate Menu. From the Alternate Menu, press the SELF TEST button. The instrument then performs the following tests:

- ROM TEST - Program Memory
- BUS TEST - Microprocessor Bus
- NVRAM TEST - Non-Volatile Battery Backed Memory
- SRAM TEST - Main Memory
- FLASH TEST - Flash Memory